


## QUANTIFICATION REPORT

### Experiment Information:

Assay Type	HBV DNA Absolute Quantification
User	360 DIAGNOSTIC
Instrument S/N	Bio-Rad CFX96™ REAL-TIME System
Run Date	10/7/2021

### QUANTIFICATION DATA FOR SAMPLE: MUKHJIT SINGH-17048

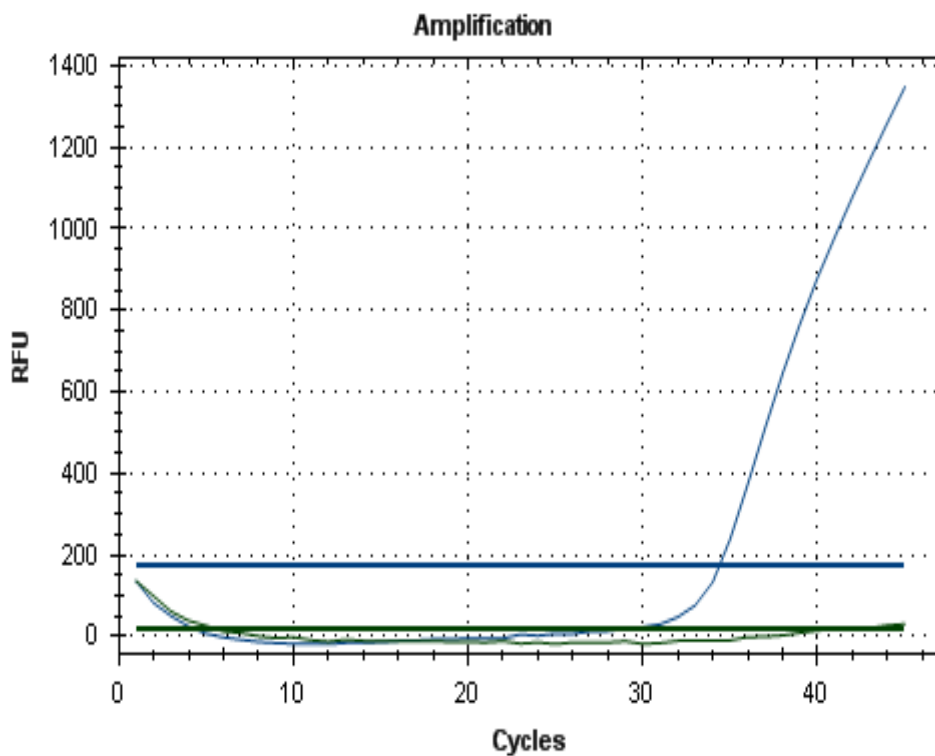

S. No.	Colour	Name	Type	Ct	Given Conc. (copies)	Calc. Conc.
1	■	MUKHJIT SINGH-10010045	HBV	34.39	NA	1506.9 U/mL
2	■	MUKHJIT SINGH-10010045	IPC	41.08	NA	NA

This report is generated by Bio-Rad™ CFX Manager IVD Edition 1.6 (Admin.)