


QUANTIFICATION REPORT

Experiment Information:

Assay Type	HBV DNA Absolute Quantification
User	
Instrument S/N	Bio-Rad CFX96™ REAL-TIME System
Run Date	17-AUGUST-21

QUANTIFICATION DATA FOR SAMPLE: MOHIT

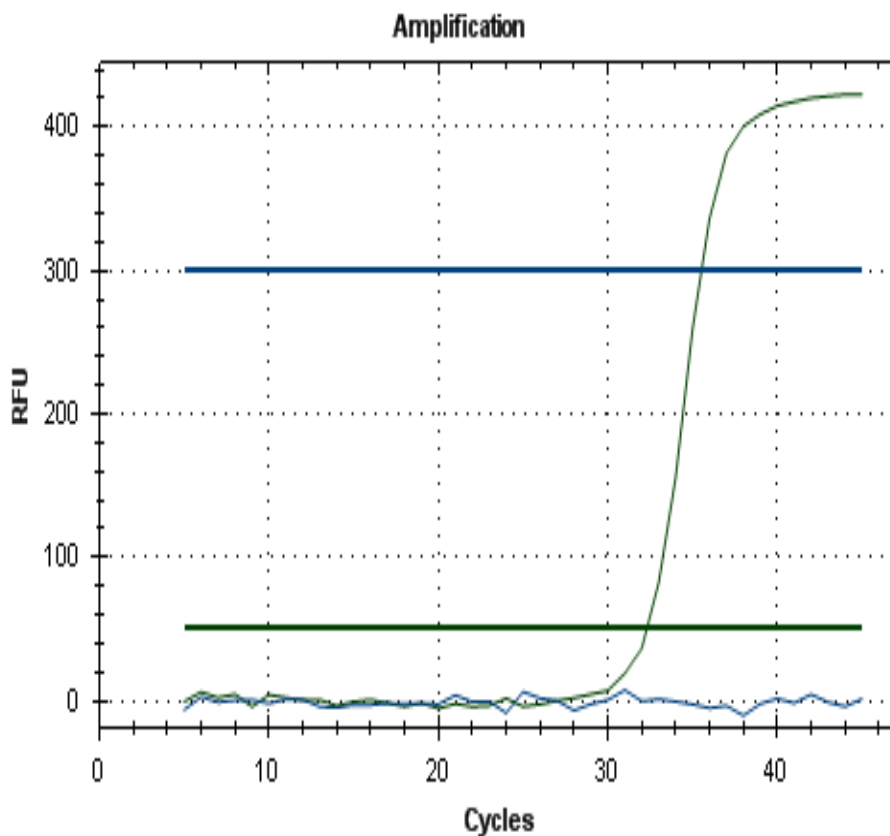

S. No	Colour	Name	Type	Ct	Given Conc. (copies)	Calc. Conc.
1	■	MOHIT	HBV	Undetermined	NA	< 50.0 IU/mL
2	■	MOHIT	IPC	32.09	NA	NA